



**GE Healthcare
Project Management**


GE Healthcare has made reasonable efforts to ensure this BIM file conforms to requirements of the applicable pre-installation manual. This BIM file was produced to assist with site planning and is not intended for construction or final building modeling. GE Healthcare is not responsible for any damages resulting from use of such file for construction or final building modeling purposes. Compliance with all applicable local, state, and federal laws and regulations is the responsibility of the customer or its designated architects and engineers. Please keep in mind the information in this BIM file is dynamic and is subject to change without notice. It is the responsibility of the customer or its designated architect(s) and engineer(s) to ensure they have the latest equipment or product information.

SINGLE PLANE INNOVA IGS 540 - RENDERING

Project number	4-68
Date	31.JAN.17
Drawn by	GENPACT
Checked by	-

A-1

Scale 12" = 1'-0"

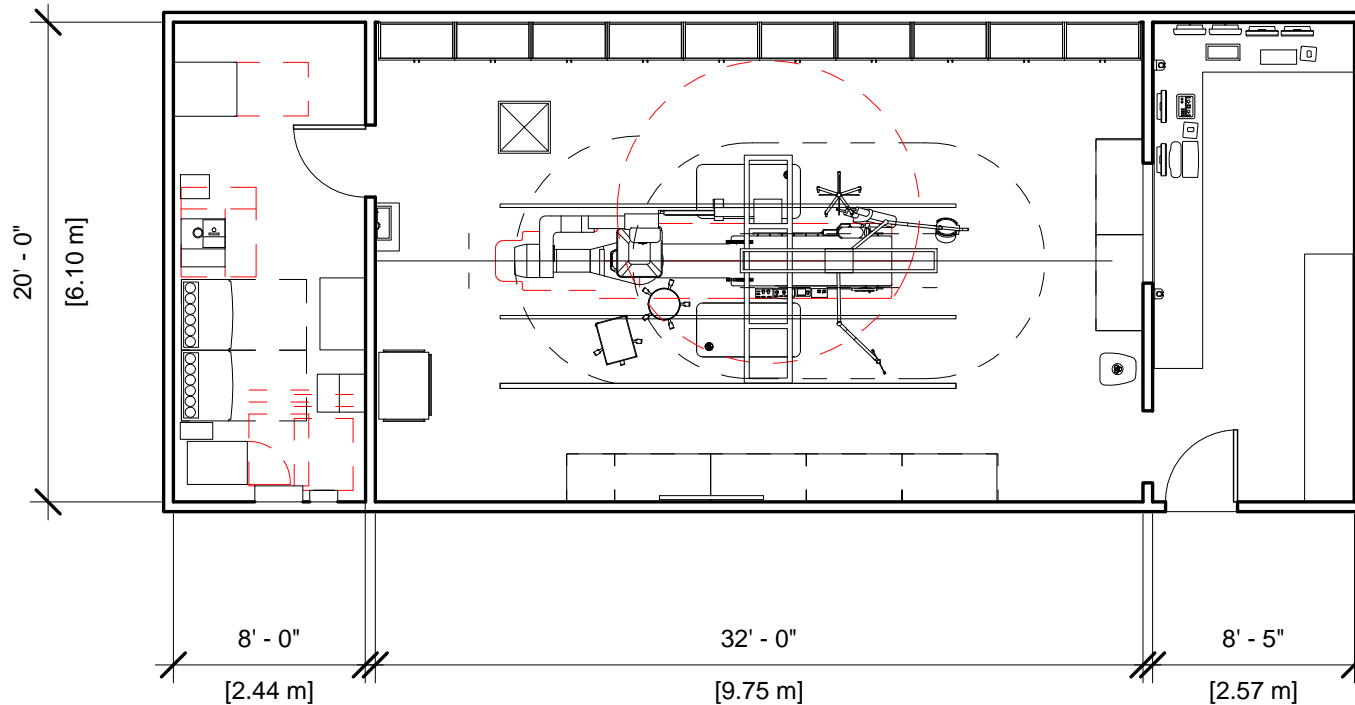

**GE Healthcare
Project Management**

GE Healthcare has made reasonable efforts to ensure this BIM file conforms to requirements of the applicable pre-installation manual. This BIM file was produced to assist with site planning and is not intended for construction or final building modeling. GE Healthcare is not responsible for any damages resulting from use of such file for construction or final building modeling purposes. Compliance with all applicable local, state, and federal laws and regulations is the responsibility of the customer or its designated architects and engineers. Please keep in mind the information in this BIM file is dynamic and is subject to change without notice. It is the responsibility of the customer or its designated architect(s) and engineer(s) to ensure they have the latest equipment or product information.

SINGLE PLANE INNOVA IGS 540 - PLAN

Project number	4-68
Date	31.JAN.17
Drawn by	GENPACT
Checked by	-

A-2

Scale 1/8" = 1'-0"

Specialty Equipment Schedule

Description	Weight (lbs)	BTU
Control Room		
BOLUS CHASE HANDSWITCH	2	0
REMOTE CONTROL FOR INJECTOR	4	0
19 in. MONITOR ON WALL SUPPORT	26	204
19 in. MONITOR ON WALL SUPPORT	26	204
OPERATORS CONSOLE WITH DL KEYPAD	22	546
OPERATORS CONSOLE	22	546
BOLUS CHASE HANDSWITCH	2	0
AW WORKSTATION	81	1201
Equipment Room		
INJECTOR ELECTRONICS	37	320
LARGE DISPLAY MONITOR CABINET	253	3412
3 KVA UPS CABINET (LARGE DISPLAY SUBSYSTEM OPTION)	99	546
CUSTOMER SUPPLIED STORAGE CABINET	0	0
150-AMP LOCAL SERVICE DISCONNECT FOR LOCK-OUT TAG-OUT CAPABILITY. (MAY BE A FUSED DISCONNECT, CIRCUIT BREAKER OR SAFETY SWITCH.)	0	0
ATLAS CABINET C2	570	1825
ATLAS CABINET C1F	1008	3389
INNOVA MAIN DISCONNECT, REFERENCE JUNCTION POINT 'PDB' ON SHEET E1 FOR DETAILED DESCRIPTION.	326	1532
DETECTOR CHILLER	33	706
COOLIX 4100 WATER CHILLER	264	18725
COOLIX 4100 AUTOTRANSFORMER	66	153
20 KVA UPS CABINET	1170	4061

Specialty Equipment Schedule

Description	Weight (lbs)	BTU
Exam Room		
CABLE DRAPE RAIL	180	0
LONGITUDINAL STATIONARY RAIL FOR LCD MONITOR	68.00	0
REMOTE CONTROL FOR INJECTOR	4	0
OMEGA IV/V TABLE WITH ROTATING TOP	1300	614
XR BUZZER (LOCATED ABOVE CEILING)	2	0
INNOVA POSITIONER	1653	2416
INJECTOR HEAD ON TABLE RAIL	15	0
COUNTERBALANCED EYE AND THYROID SHIELD WITH R96 LAMP	143	0
LARGE DISPLAY MONITOR ON SINGLE MONITOR SUSPENSION 9 ft. 6 in. INBOARD BRIDGE (MOUNT TWO GE MONITORS ON BACKSIDE OF LD MONITOR)	784	1706



**GE Healthcare
Project Management**

GE Healthcare has made reasonable efforts to ensure this BIM file conforms to requirements of the applicable pre-installation manual. This BIM file was produced to assist with site planning and is not intended for construction or final building modeling. GE Healthcare is not responsible for any damages resulting from use of such file for construction or final building modeling purposes. Compliance with all applicable local, state, and federal laws and regulations is the responsibility of the customer or its designated architects and engineers. Please keep in mind the information in this BIM file is dynamic and is subject to change without notice. It is the responsibility of the customer or its designated architect(s) and engineer(s) to ensure they have the latest equipment or product information.

SINGLE PLANE INNOVA IGS 540 - SCHEDULE

Project number	4-68
Date	31.JAN.17
Drawn by	GENPACT
Checked by	Checker

A-3

Scale

Hold the Left Click for Rotating around
Use the Scroll for Zooming in and out



Single Plan Innova IGS 540



GE Healthcare

[Click for Site Planning Support](#)